
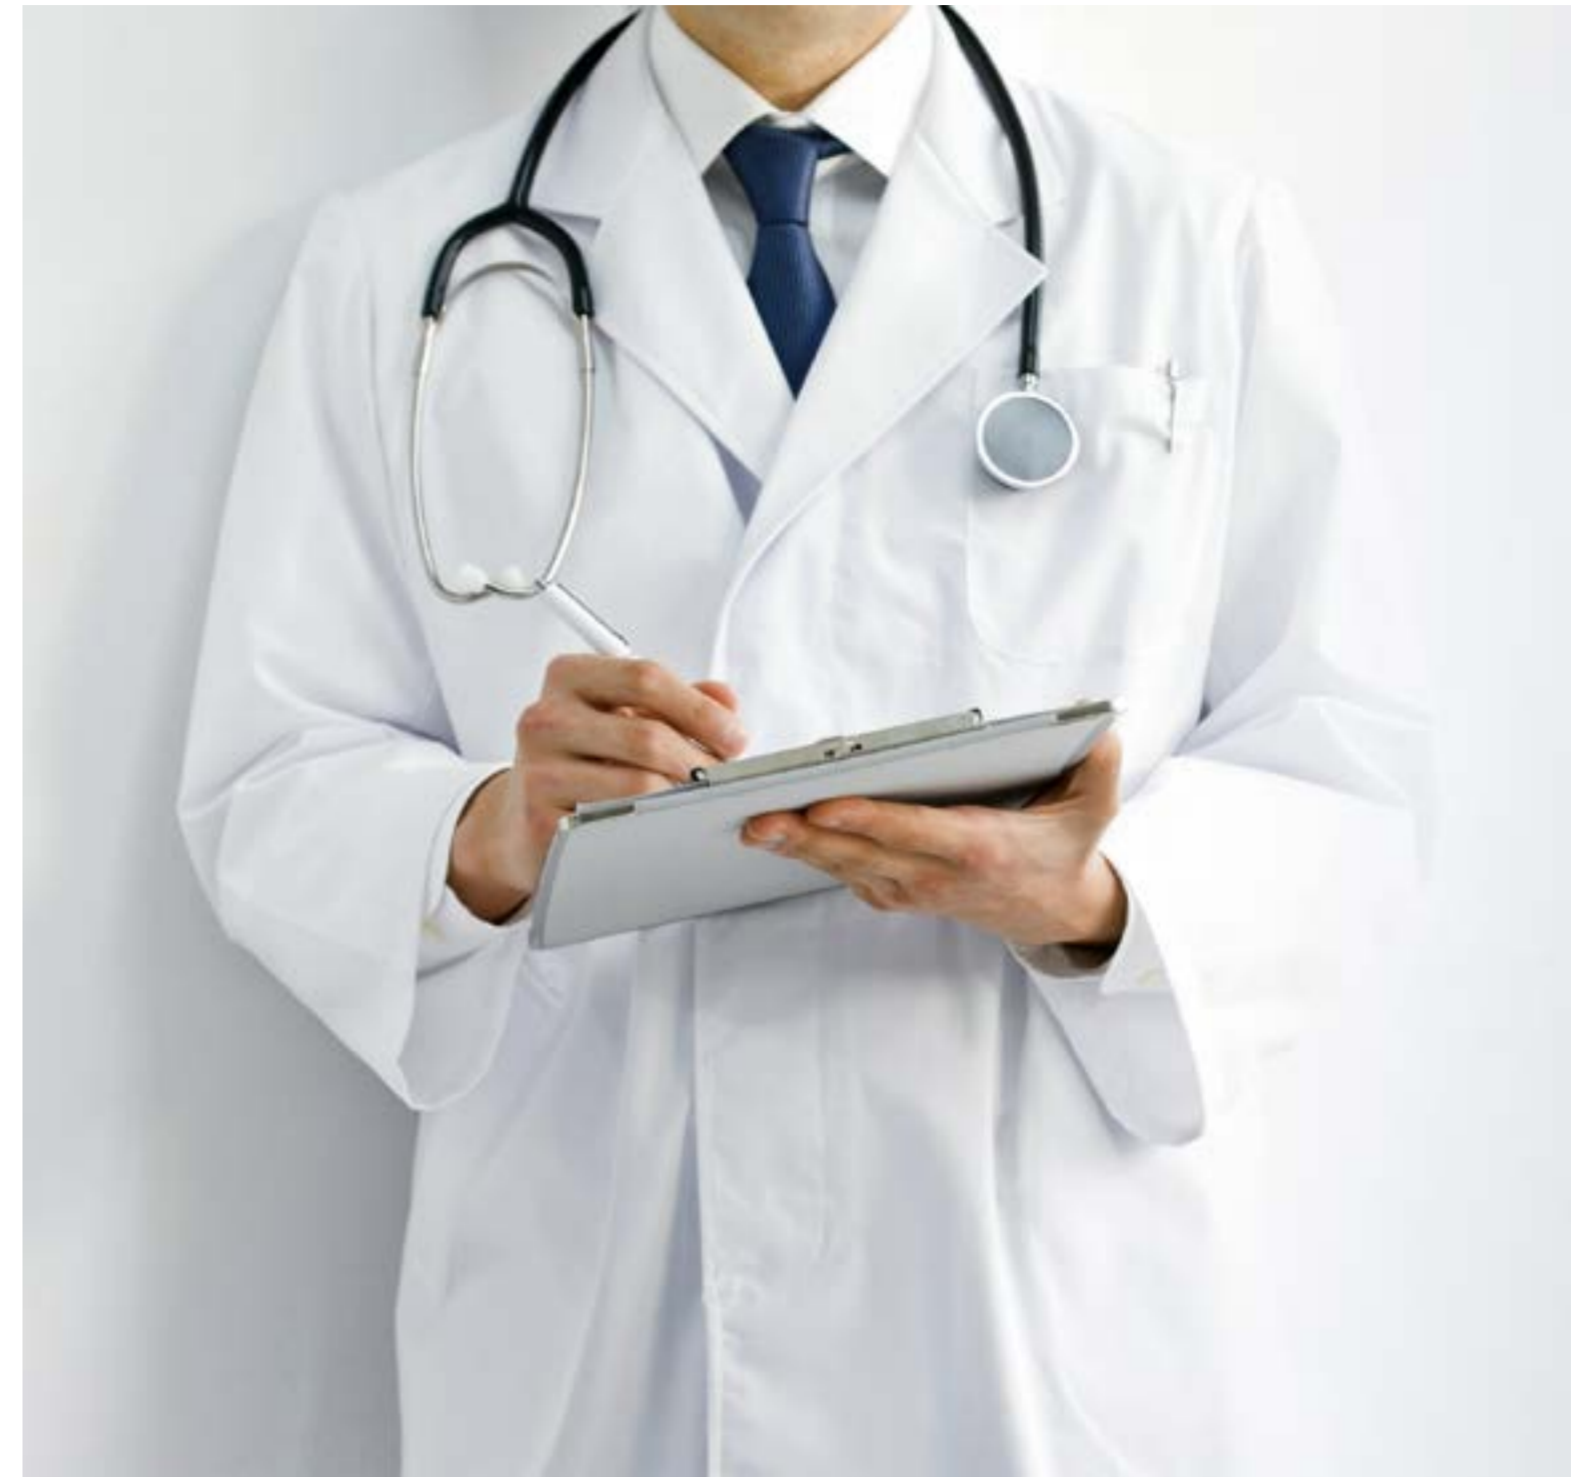


Actreen SafeSet®

	CH	234 210	234 218
ACTREEN SAFESSET® Nelaton 47 cm			
	10	234 210	50
	12	234 212	50
	14	234 214	50
	16	234 216	50
	18	234 218	50



Hur fungerar det?

ACTREEN SAFESSET®

DIN PARTNER FÖR PREVENTION AV
SJUKHUSRELATERADE INFEKTIONER

3ZcRf_ > VUZTRJ 23 mDg@Ug@XV_ # " m) # " # 5R_LWj U
hhhZScRf_žV

The content of this document, in particular the data, the information, the trademarks and the logos are B BRAUN MEDICAL SAS's sole property and are protected under copyright ©2013, B BRAUN MEDICAL, all rights reserved. Consequently, all representation and/or reproduction, whether in part or in full, is forbidden and would be considered a violation of B BRAUN MEDICAL SAS's copyright and other proprietary rights.

The products commercialized by B BRAUN MEDICAL shall exclusively be used in accordance with the package inserts which have been updated and included in the boxes.

For healthcare professional use
Ref: Z600729 06/2017

Actreen SafeSet®

© Veed Ved ^ © WdUZe Ree R_g®_UR WcfcZ \ReVedZVcZ_X a⁻
 d[f \Yf dVed^ VUV_Z_eVXdVdRU _]WZac geRX_Z_Xda` æV/c
 fcZ_ac` gZ

○ :_eVXdVdRU _]WZac` geRX_Z_Xda` æV/c Ree
 ^` egVc\R \c` dd \ontamination


Stängt system – Allt i ett

<ReVedc` _TY a`dV_dZæVcZ` a` TY
 X`cZ_eV/Ree` \aa]R_ZW`_gRcR_UcZ



A`]Ze]Z UZR`_` d gZ\Ve ^ ;]ZXZc
 S@eeV R_eSZ eZd\ SVYR_U]Z_X


=®^ a]Z Ree R_g®_UR Z` a ^ WU`]ZR ej aVcRg
 fcZ_ac` geRX_Z_XdR` dU_Z_XRc

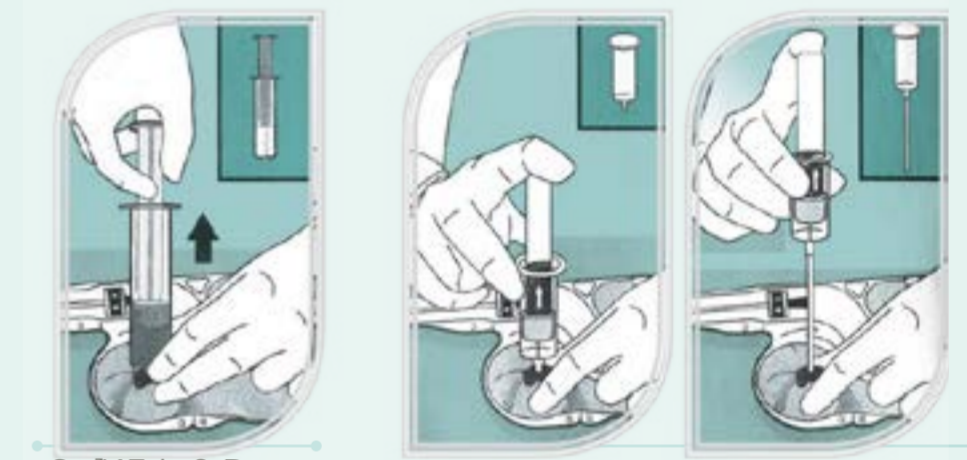

?`]WZchcf eZ
 =fVd` aa]Z_X

GRVf ^ q dV^

**B. BRAUN
 PATENT**

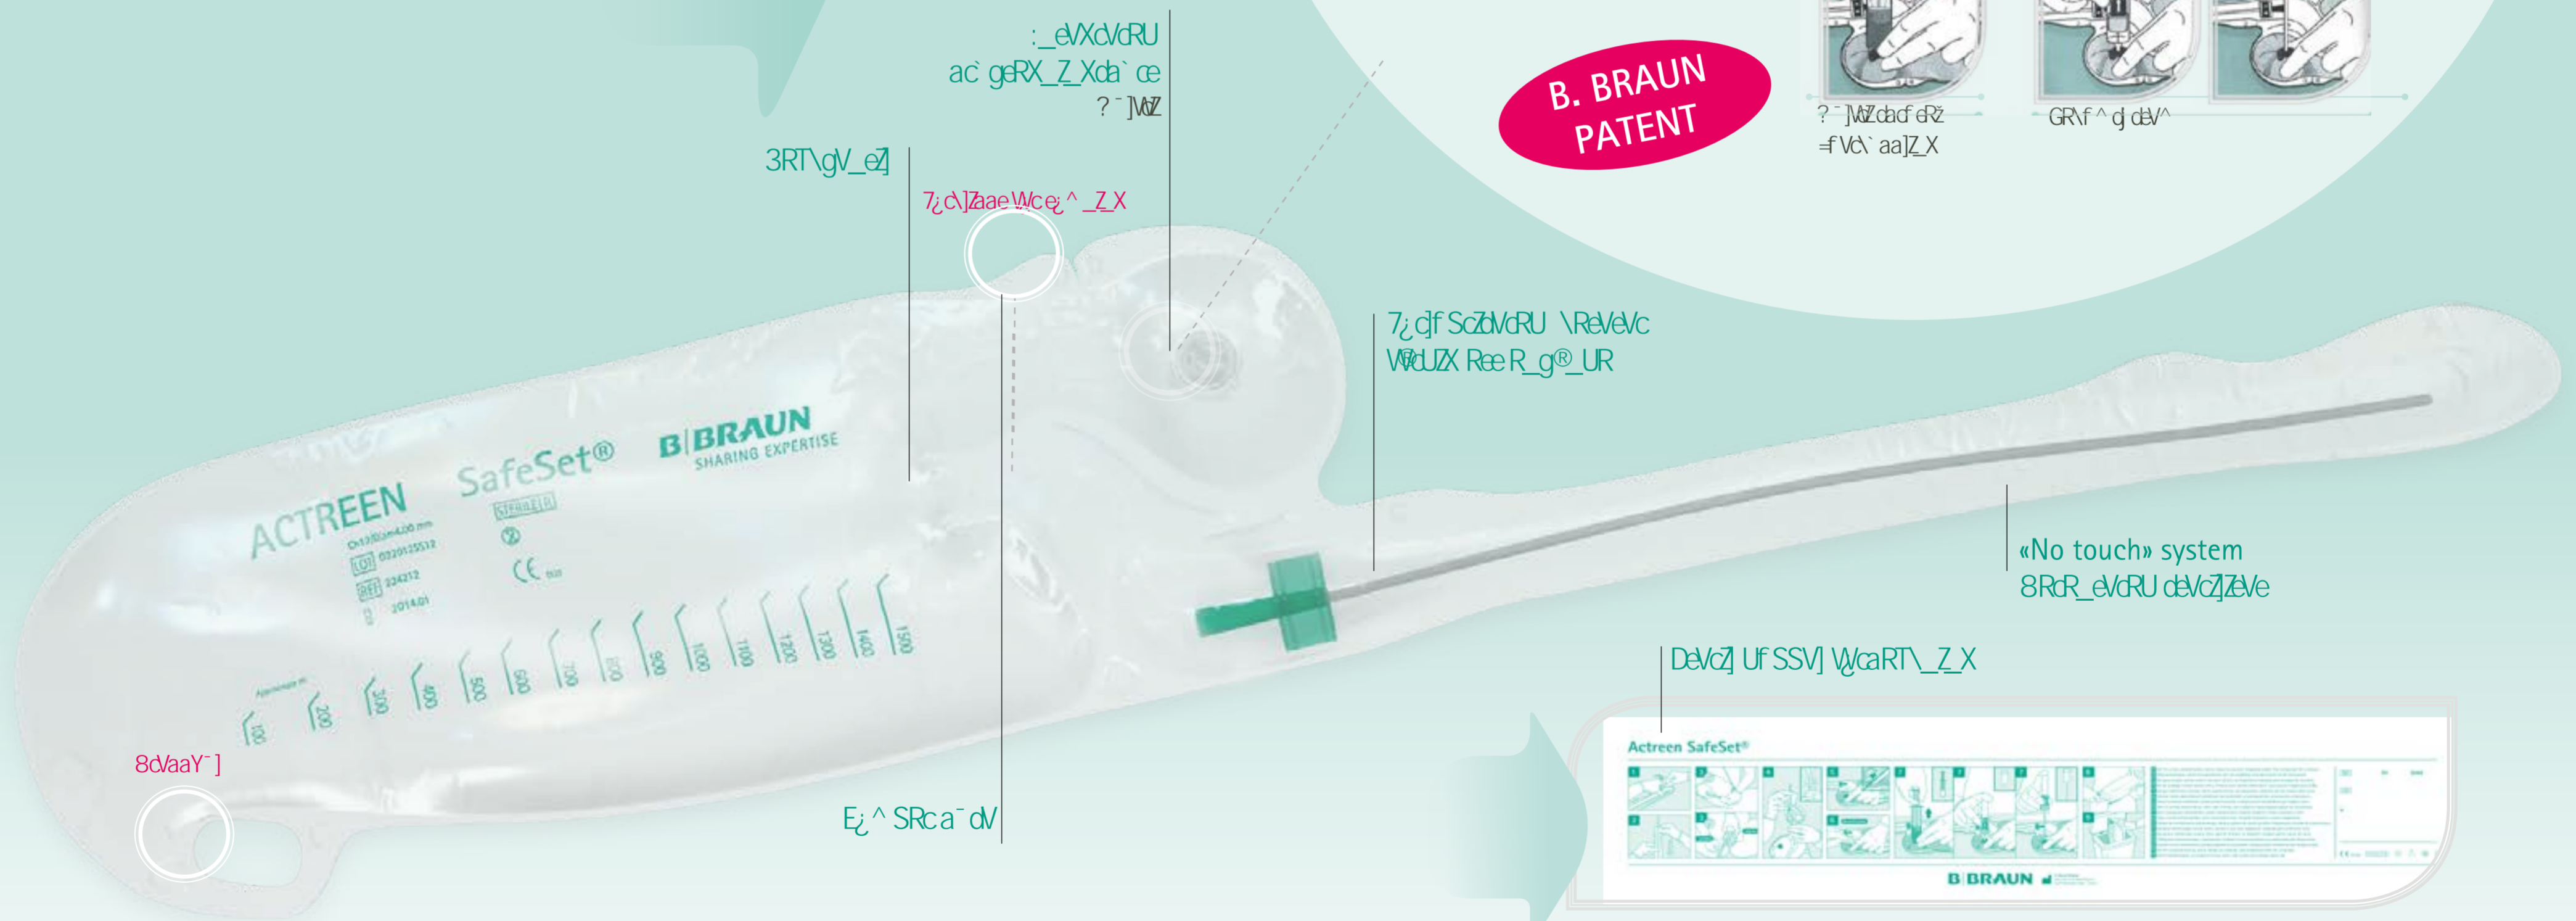

:_eVXdVdRU
 ac` geRX_Z_Xda` æ
 ?`]WZ

3RT\gV_e]

7; d]ZæeWce^ _Z_X

7; df ScZVdRU \ReVedc
 WdUZe Ree R_g®_UR

«No touch» system
 8RcR_eVcRU dæVcZæVe

DæVc] Uf SSV] WcaRT`_Z_X

8d/aaY`]

E; ^ SRca` dV



FÖRBEREDELSE
1
KATETRISERING

- 7; cSVdUMdV Rg aReV_e
 - 9R_UUdZ WaeZ
 - CV_X; cZ_X Rg XV_ZRJR
- 3; cf eWdV_JXeVce
Z^a]V^V_eVdRUU ac e \]]

1. Eaa RUV dēvZIR
WcaRT\ ZXV XV ^ ReecZgR
Rg LaWJa dV_U TY R_g® U
UV d ^ V dēvZ UdRavcZ_X
f_Uvcac TVUf dV_



2. 7; c Ree WZ; dR \ReVe/cdaVedV_c
;aa_R gZU ^ @cV 2 Wc Ree
R_g® UR U^ te fTYUd dēv^ VeZ
@^ _UF_gZ] WZ; dR YVJR
\ReVe/c_cZg Rg gZU ^ @cVe4Z
**Katetern är för-lubricerad och
färdig att använda.**



3. 7 cedRe \ReVe/cZ XV
fER_ ReegZUc dR \ReVe/c_Z
ER fe \ReVe/c_ @cfz_ dJf dRe
WUR_Z_ZfcZ_a dV_Z



FÖRBEREDELSE
2
URINPROVTAGNING

4. E]WcfzV_eZ] e aaV_Rg
a dV_XV_ ^ ReUdRfaa
a dV dS^ eV_WcReeWJR
^ c UvegZU
ac gRX_Z Xda` cēV ^ WU
f cZ_Z



5. E]T\ a^ ac gRX_Z Xd
a` cēV_WcReef_UgZAR
]f WsfSS] cf_UVcZ



6. 5VdZ WIVcR
ac gRX_Z Xda` cēV
WdV f cZ ac gRX_Z XZ



URINPROVTAGNING

7. 7; cZ_fē] aaVeZac gRX_Z Xda` cēV_Z
7 cedRe ac gRX_Z XV_V]XeZ daf`VeZ _VcWcUW_
ac Uf\ eUf R_g®_UvcZ



> WU_]WZ
daf eRZ]f Vc

> WU
gRf^ d dēV^



CVU Wc
f cZ_R_R]j d

8. Cz Rg gZU ^ R cVcZ X5 Wc
Ree WZ; dR ^ c UvegZU
ac gRX_Z Xda` cēV TY Wc
Ree^ ^ Ra dV_Z

